# **DentaKLEEN**®

### WATERLINE CLEANING SYSTEM FOR DENTAL UNITS ON CITY WATER

ITEM #: MAK-1900

### **INSTALLATION GUIDE**

#### **STEP 1: PREPARE FOR INSTALLATION**

- 1. Turn Dental Unit OFF.
- 2. Confirm that no Air or Water comes out of the 3-Way Syringe.

#### STEP 2: MOUNTING DentaKLEEN® SYSTEM

- 1. Identify a Location to Mount on a Vertical 2" Light Post or a Flat Surface.
- 2. The Location should be as close as possible to the Dental Unit's Internal Tubing of Air and Water Supply.


#### **STEP 3: MAKING THE CONNECTIONS**

- 1. On the Dental Unit, Locate a 1/8" Air Line (Yellow) Connected to the Dental Unit's ON/OFF Switch.
- 2. Confirm the ON/OFF Switch is a 3-Way Switch.
- 3. Cut this Yellow Air Line and "T" to the DentaKLEEN® SYSTEM's Air Line.
- 4. On the Dental Unit, Locate a 1/4" Waterline (Blue); Cut this Blue Waterline and "T" the DentaKLEEN® SYSTEM to this Line.

#### **STEP 4: OPERATION CHECK**

- 1. Turn Water and Air **ON** at Dental Unit's Junction Utility Box.
- 2. Turn Dental Unit **ON** and Check for Air and Water Leaks.

## DentaKLEEN®

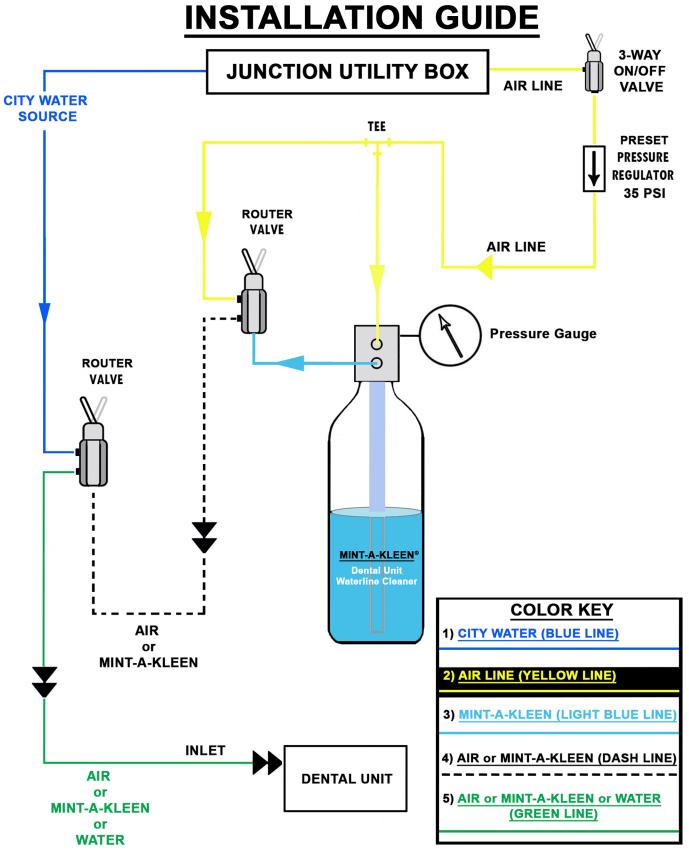

Anodia Systems, LLC, Dental Manufacturer 109 Larrimore Lane | Danville, KY 40422 USA P: 866.246.2548 | E: info@AnodiaSystems.com www.AnodiaSystems.com